

ZytoDot 2C CEN X/Y Probe

REF C-3048-400

$\nabla \Sigma$ 40 (0.4 ml)


For the detection of human alpha-satellites of
chromosome X and chromosome Y by chromogenic
in situ hybridization (CISH)



IVD

In vitro diagnostic medical device

according to EU directive 98/79/EC

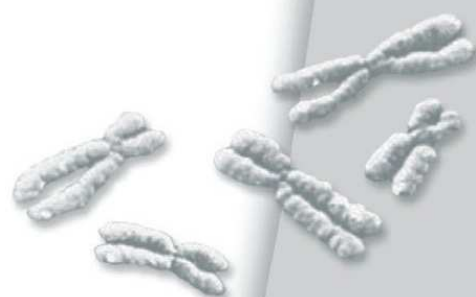

Digoxigenin and DNP labeled polynucleotide probe for the detection of human chromosome X and chromosome Y alpha-satellites by CISH, ready to use

Product Description

- Content:** ZytoDot 2C CEN X/Y Probe (PD28) in hybridization buffer. The probe contains DNP-labeled polynucleotides, which target alpha-satellite-sequences of the centromere of chromosome X and digoxigenin-labeled polynucleotides, which target alpha-satellite-sequences of the centromere of chromosome Y.
- Product:** C-3048-400: 0.4 ml (40 reactions of 10 µl each)
- Specificity:** ZytoDot 2C CEN X/Y Probe (PD28) is designed to be used for the detection of chromosome X as well as of chromosome Y alpha-satellites in formalin-fixed, paraffin-embedded tissue or cells by chromogenic *in situ* hybridization (CISH).
- Storage/Stability:** The ZytoDot 2C CEN X/Y Probe (PD28) must be stored at 2...8°C and is stable through the expiry date printed on the label.
- Use:** This product is designed for *in vitro* diagnostic use (according to EU directive 98/79/EC). Interpretation of results must be made within the context of the patient's clinical history with respect to further clinical and pathologic data of patient by a qualified pathologist!
- Safety Precautions:** Read the operating instructions prior to use!
- Do not use the reagents after the expiry date has been reached!
- This product contains substances (in low concentrations and volumes) that are harmful to health. Avoid any direct contact with the reagents. Take

appropriate protective measures (use disposable gloves, protective glasses, and lab garments)!

If reagents come into contact with skin, rinse skin immediately with copious quantities of water!

A material safety data sheet is available on request for the professional user!

Principle of the Method

The presence of certain nucleic acid sequences in cells or tissue can be detected by *in situ* hybridization using labeled DNA probes. The hybridization results in duplex formation of sequences present in the test object with the labeled DNA probe.

Duplex formation of the labeled probe (with sequences of chromosome X and chromosome Y alpha-satellites in the test material) can be visualized using primary (unmarked) antibodies, which are detected by secondary polymerized enzyme-conjugated antibodies. The enzymatic reactions of chromogenic substrates lead to the formation of colored signals that can be visualized by light microscopy.

Instructions

Pre-treatment (dewaxing, proteolysis, post-fixation) should be carried out according to the needs of the user.

Denaturation and hybridization of probe:

1. Vortex the ZytoDot 2C CEN X/Y Probe (PD28) and pipette 10 µl each onto individual samples

Distribute dropwise on the whole target area to avoid local concentration of probe. Alternatively, add probe to the center of a coverslip and place it upside down on target area. A gentle warming of the probe, as well as using a pipette tip, which has been cut off to increase the size of the opening, can make the pipetting process easier.

2. Avoiding trapped bubbles, cover the samples with a coverslip (22 mm x 22 mm). Seal the coverslip, e.g. with a layer of hot glue from an adhesive pistol or with rubber cement

3. Denature the slides at 78-80°C for 5 min, e.g. on a hot plate

4. Transfer the slides to a humidity chamber and hybridize overnight at 37°C (e.g. in a hybridization oven)

It is essential that the tissue/cell samples do not dry out during the hybridization step.

Further processing, such as washing, detection, and counter-staining, can be completed according to the user's needs. For a particularly user-friendly performance, we recommend the use of a ZytoDot 2C CISH system by ZytoVision. These systems were also used for the confirmation of appropriateness of the ZytoDot 2C CEN X/Y Probe (PD28).

Results

In an interphase nucleus of normal male cells or male cells without aberrations of chromosome X and Y, one chromosome X and one chromosome Y specific punctual signal appears which can be clearly distinguished from the background. In an interphase nucleus of normal female cells or female cells without aberrations of chromosome X, two chromosome X signals appear (color and appearance of the signals depend on the detection system that is used). In cells with an aneuploidy of chromosome X or Y, a different signal pattern is visible in interphases.

Due to mitosis, additional signals may be visible in a small percentage of cells. Occasionally, nuclei with missing signals may be observed in paraffin-embedded tissue sections.

In order to judge the specificity of the signals, every hybridization should be accompanied by controls. We recommend using at least one control sample in which the chromosome X and chromosome Y copy number is known.

Our experts are available to answer your questions.

Literature

- Coussens L, et al. (1985) *Science* **230**: 1132-9.
- Isola J, Tanner M (2004) *Methods Mol Med* **97**: 133-44.
- Mayr D, et al. (2009) *Histopathology* **55**: 716-23.
- Nakahori Y, et al. (1986) *Nucleic Acids Res* **14**: 7569-80.
- Speel EJ, et al. (1994) *J Histochem Cytochem* **42**: 1299-307.
- Tsukamoto T, et al. (1991) *Int J Dev Biol* **35**: 25-32.
- Waye JS, Willard HF (1987) *Nucleic Acids Res* **15**: 7549-69.
- Wilkinson DG: In Situ Hybridization, A Practical Approach, *Oxford University Press* (1992)
ISBN 0 19 963327 4.

As of: March 1, 2011 (5.0)

Trademarks:

ZytoVision® and ZytoDot® are trademarks of ZytoVision GmbH.



ZytoVision GmbH · Fischkai 1
D - 27572 Bremerhaven · Germany
Phone: +49 (0)471/4832 - 300
Fax: +49 (0)471/4832 - 509
www.zytovision.com
info@zytovision.com



Your local distributor